



AAA DENTALAB

1st Floor, Unit 4 Watling Gate,
297-303 Edgware Road,
London NW9 6NB.

www.aaadentalab.co.uk

✉ : infouk@aaadentalab.com

☎ : 0203 6022728

☎ : 07400066241

Impression

Date :

Date

Required:

1 working day before actual appointment

Dentist

Name:

Practice Name :

Postcode (Acc No.):

Patient ID / Code :

☐ Male

☐ Female

D.O.B.:

**We Accept
All Digital
Scan**



Restoration Type

- ☐ Cement Retained
☐ Screw Retained
☐ Single Unit Crown (s)
☐ Multi Unit Bridge

Implant Abutment(s)

- ☐ Custom Abutment(s)
☐ Stock Abutment(s)

Components Enclosed

- ☐ Abutment
☐ Analogur
☐ Lab Screw
☐ Other

Porcelain Fused Metal

- ☐ Non-Precious
☐ Semi-Precious
☐ Precious

Metal Free Ceramics

- ☐ Composite
☐ Full Zirconia
☐ Zirconia with Emax® Layering
☐ Emax® Press


If Insufficient Room

- ☐ Metal Occlusion
☐ Adjust Opposing

I have disinfected the impression :

With :

By :

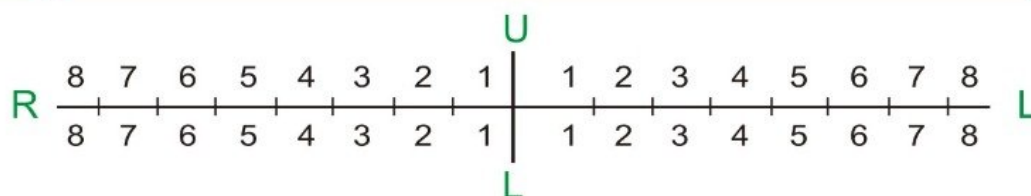

Special Instructions:

Shade

Vita Classic

Lab use only :

THIS DEVICE IS NON STERILE

(Full Terms & Conditions are attached with our pricelist or visit our web at www.aaadentalab.co.uk) MHRA No. 8496/GDC No. 285519 / DLA MEMBER
Your attention is drawn to the following statement: This is a custom-made dental device that has been manufactured to satisfy the design characteristics, properties and detail of what has been prescribed by the above dentist. This dental device is purely manufactured for exclusive use of the patient described above. The product meets the general safety and performance requirements specified in the Annex I of Medical Devices Regulations. This product may have been produced in either or both UK and China by AAA Dentalab LTD.

Instructions for use, storing & handling : It is highly recommended that, this dental device is stored in a clean and safe environment that prevents it from coming in contact with materials, liquids or acids that could cause disfiguration or damage to the dental device. The dental device should not be subjected to extreme heat. Where applicable, you should take care not to damage the dental device(s) when removing from its model.

Prescriber Feedback: To enable our dental laboratory to comply with the Medical Devices Regulations for Post Market Surveillance, please inform us of any feedback or issues regarding the enclosed device(s) as soon as possible.